


Lab Notebook Entry from LeCroy DSO  
DSO S/N: LCRY4203N20379  
User: LeCroyUser  
Time: 4/24/2019 7:45:53 AM

1.2v dvcc noise at 1MHz BW--00000



## LabNotebook

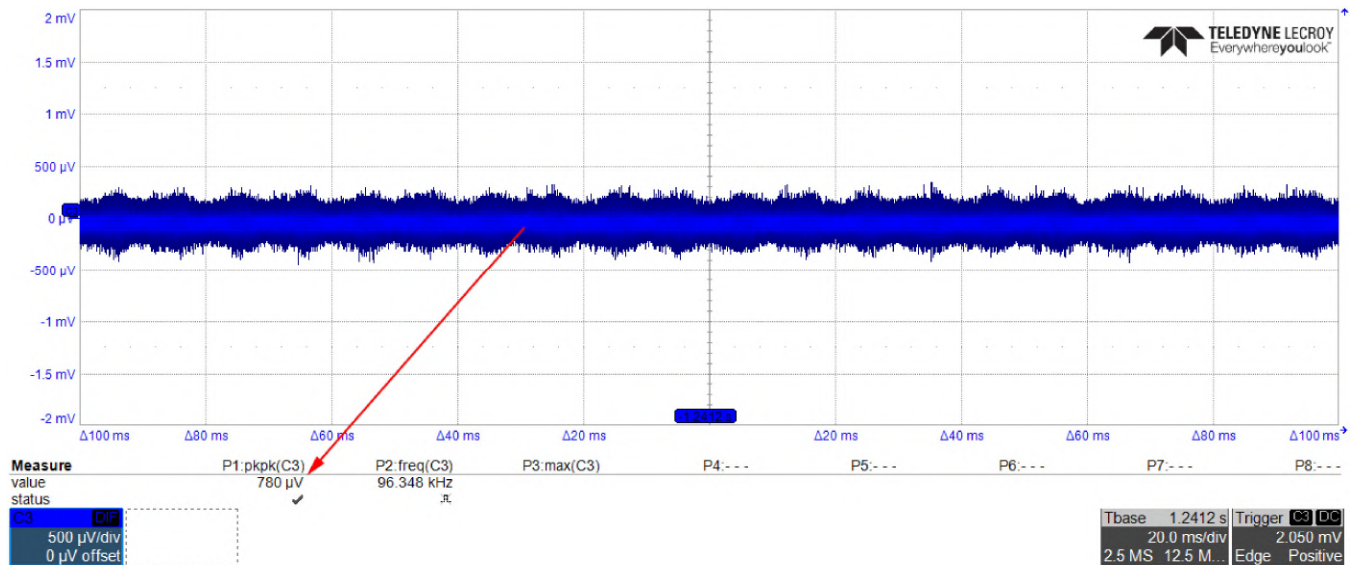

### Channel Status

		C3
Vertical	V / Div	500 $\mu$ V
	Offset	0 $\mu$ V
	Coupling	DC50 $\Omega$
	BW-Limit	1GHZ
	Probe	100.000e-3
	Sweeps	1 #

### Acquisition Status

Horizontal	Time / Div	20.0 ms	Sampling Rate	12.500000 MS/s
	Time / Pt	80.000000 ns	Sampling Mode	RealTime
	Pts / Div	250.0000 kS	Trigger Delay	1.2412 s
Trigger	Mode	Stop	Slope	Positive
	Type	Edge	Level	2.050 mV
	Source	C3	Coupling	DC