


Lab Notebook Entry from LeCroy DSO
DSO S/N: LCRY4203N20379
User: LeCroyUser
Time: 7/7/2017 5:05:44 AM

7/7/2017 5:05:44 AM

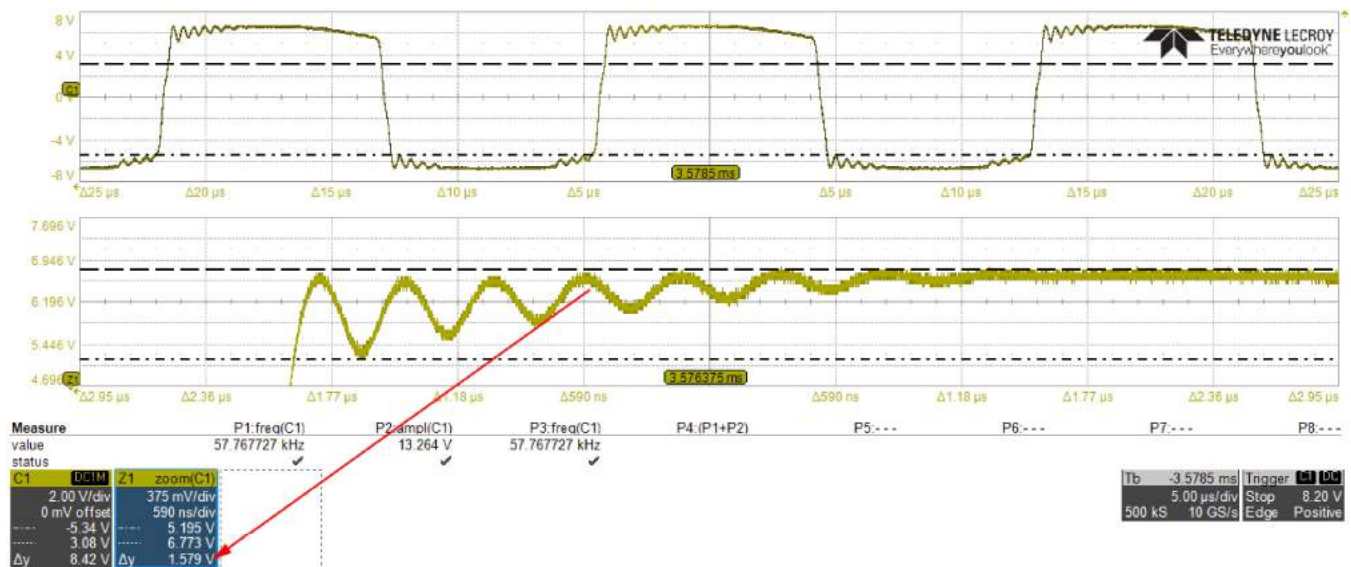

Channel Status

| | | |
|----------|----------|--------|
| | | C1 |
| Vertical | V / Div | 2.00 V |
| | Offset | 0 mV |
| | Coupling | DC1MΩ |
| | BW-Limit | 1GHZ |
| | Probe | 10 |
| | Sweeps | 1 # |

Acquisition Status

| | | | | |
|------------|------------|------------|---------------|-------------------|
| Horizontal | Time / Div | 5.00 μs | Sampling Rate | 10.000000000 GS/s |
| | Time / Pt | 100.000 ps | Sampling Mode | RealTime |
| | Pts / Div | 50.0000 kS | Trigger Delay | -3.5785 ms |
| | Mode | Stop | Slope | Positive |
| Trigger | Type | Edge | Level | 8.20 V |
| | Source | C1 | Coupling | DC |