


Lab Notebook Entry from LeCroy DSO
DSO S/N: LCRY4203N20379
User: LeCroyUser
Time: 12/11/2017 10:16:17 PM

diode osc affter 2pf cap time--00000



LabNotebook

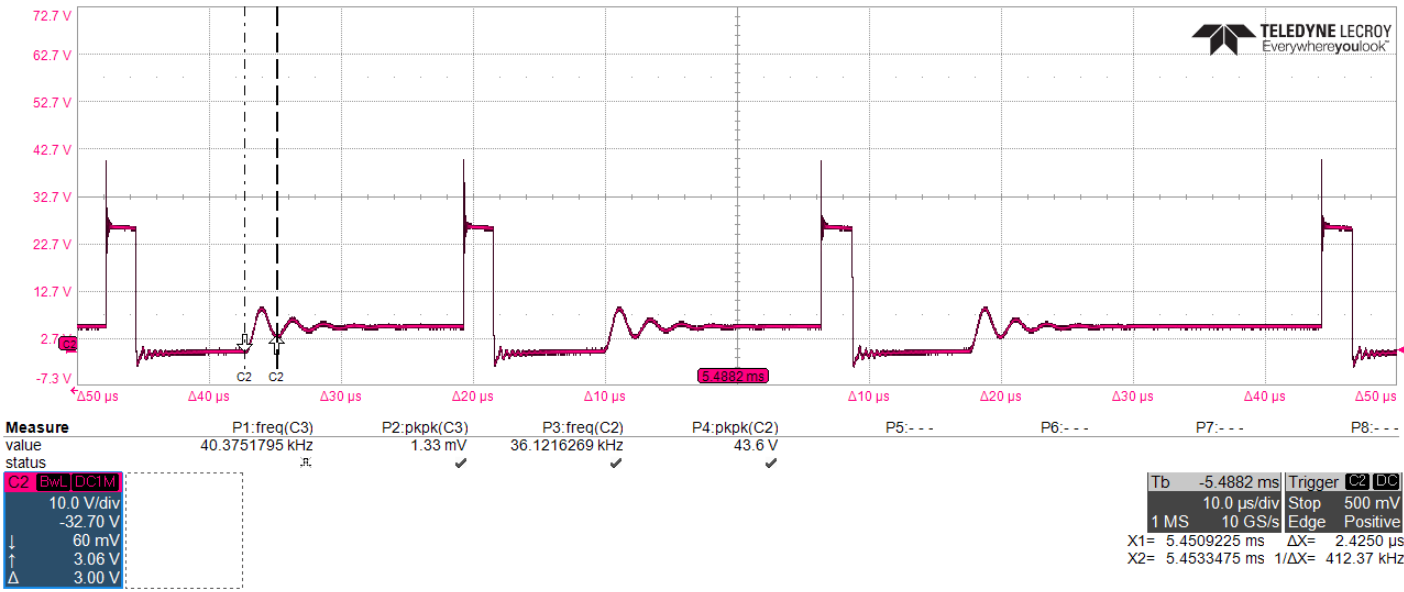

Channel Status

	C2	C3
V / Div	10.0 V	2.00 mV
Offset	-32.70 V	0 μV
Coupling		
BW-Limit		
Probe		
Sweeps	1 #	1 #

Acquisition Status

	Time / Div	10.0 μs	Sampling Rate	10.00000000 GS/s
Horizontal	Time / Pt	100.000 ps	Sampling Mode	RealTime
	Pts / Div	100.0000 kS	Trigger Delay	-5.4882 ms
	Mode	Stop	Slope	Positive
Trigger	Type	Edge	Level	500 mV
	Source	C2	Coupling	DC