


Lab Notebook Entry from LeCroy DSO
DSO S/N: LCRY4203N20379
User: LeCroyUser
Time: 8/26/2019 3:17:53 AM

DVCC 1.2V_AXIS at 1MHz--00000



Lab Notebook

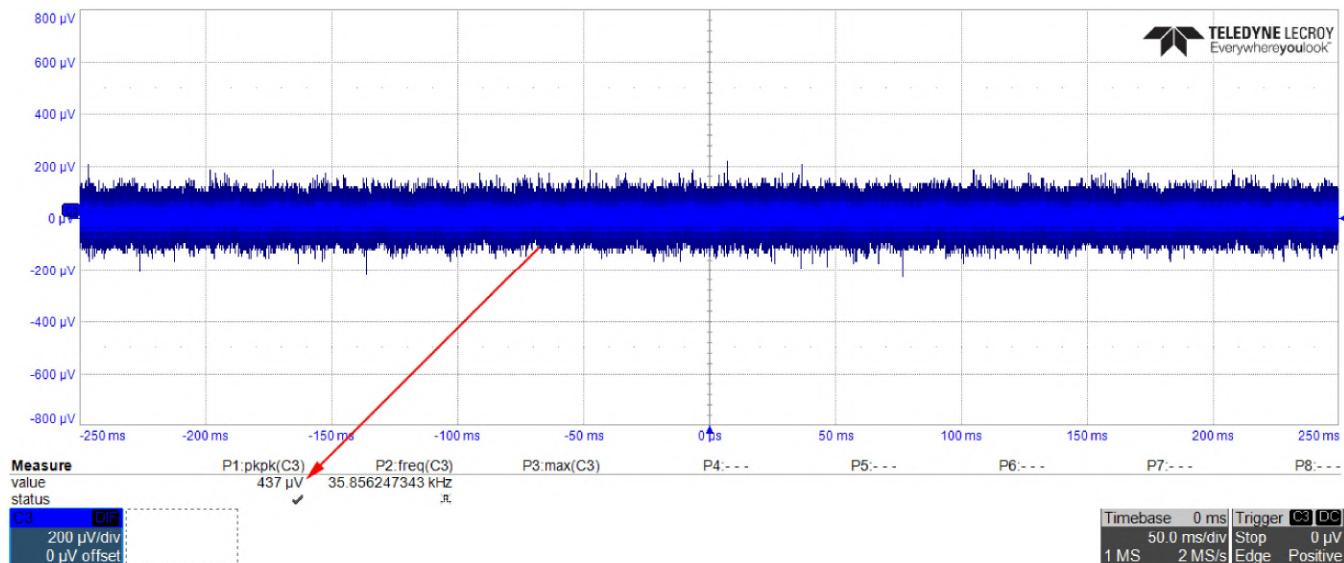

Channel Status

| | | C3 |
|----------|----------|------------|
| Vertical | V / Div | 200 μV |
| | Offset | 0 μV |
| | Coupling | DC50Ω |
| | BW-Limit | 1GHZ |
| | Probe | 100.000e-3 |
| | Sweeps | 1 # |

Acquisition Status

| | | | | |
|------------|------------|---------------|---------------|---------------|
| Horizontal | Time / Div | 50.0 ms | Sampling Rate | 2.000000 MS/s |
| | Time / Pt | 500.000000 ns | Sampling Mode | RealTime |
| | Pts / Div | 100.0000 kS | Trigger Delay | 0 ms |
| Trigger | Mode | Stop | Slope | Positive |
| | Type | Edge | Level | 0 μV |
| | Source | C3 | Coupling | DC |