


Lab Notebook Entry from LeCroy DSO
DSO S/N: LCRY4203N20379
User: LeCroyUser
Time: 5/26/2017 2:55:35 AM

5/26/2017 2:55:35 AM

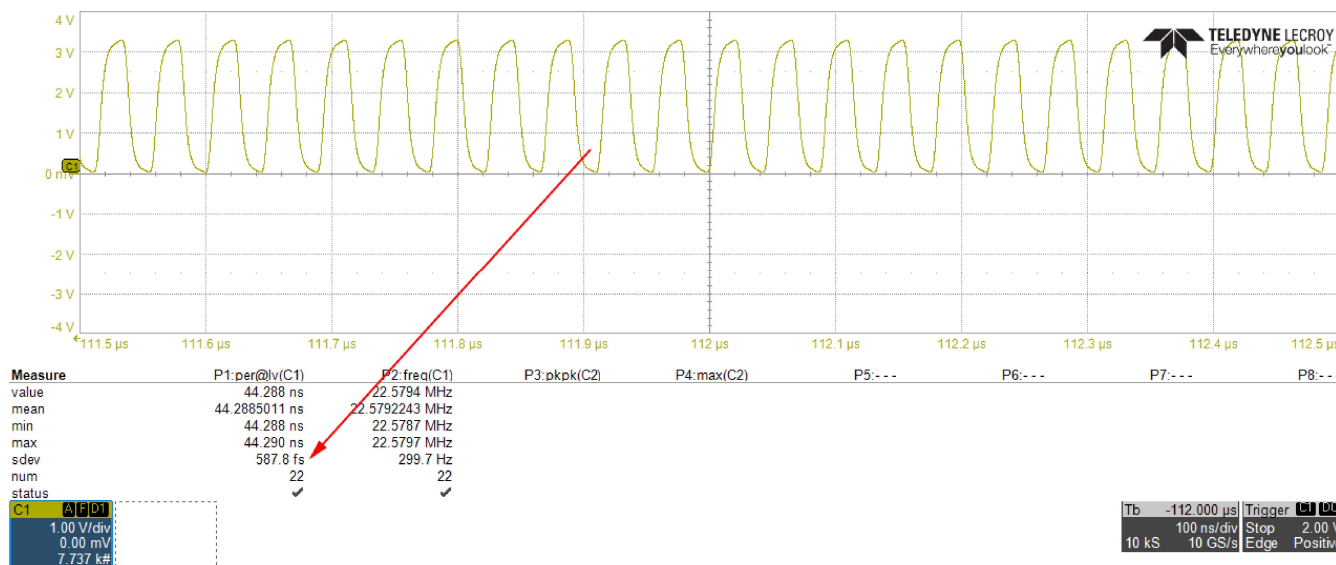

Channel Status

C1	
V / Div	1.00 V
Offset	0.00 mV
Coupling	DC1MΩ
BW-Limit	1GHZ
Probe	10
Sweeps	7.737 k#

Acquisition Status

Horizontal	Time / Div	100 ns	Sampling Rate	10.000000000 GS/s
	Time / Pt	100.000 ps	Sampling Mode	RealTime
	Pts / Div	1.0000 kS	Trigger Delay	-112.000 μs
	Mode	Stop	Slope	Positive
Trigger	Type	Edge	Level	2.00 V
	Source	C1	Coupling	DC