


Lab Notebook Entry from LeCroy DSO
DSO S/N: LCRY4203N20379
User: LeCroyUser
Time: 5/17/2018 7:02:57 PM

output ripple 1MHz ripple and noise1A load -00001--00000

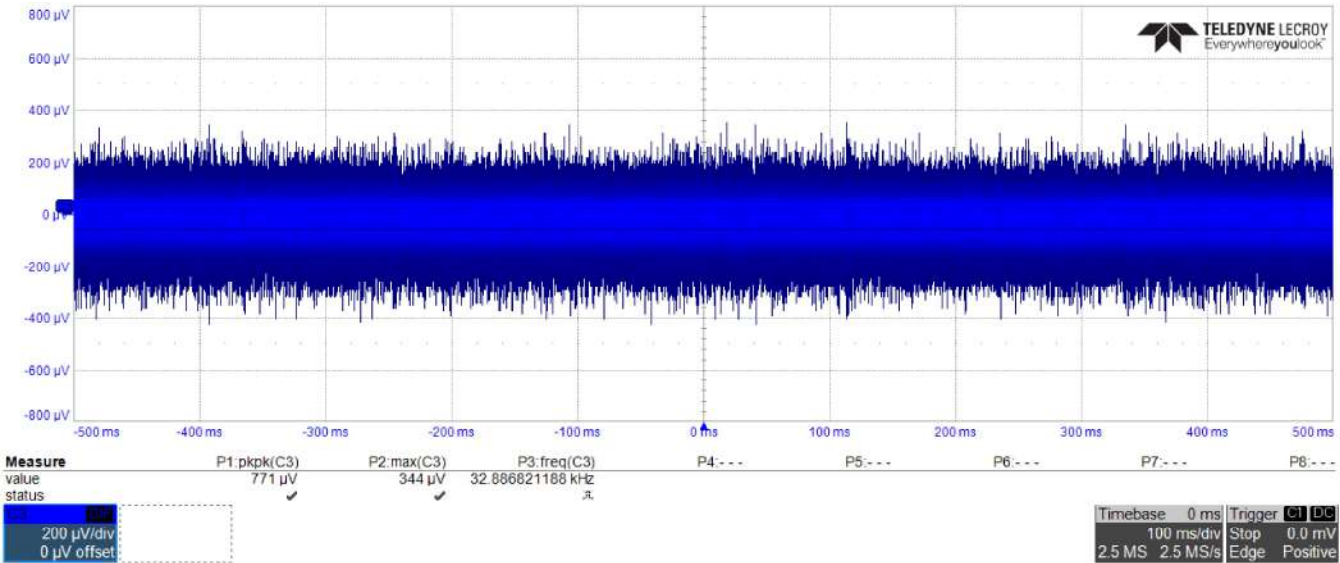

Channel Status

		C3
Vertical	V / Div	200 μV
	Offset	0 μV
	Coupling	DC50Ω
	BW-Limit	1GHZ
	Probe	100.000e-3
	Sweeps	1 #

Acquisition Status

Horizontal	Time / Div	100 ms	Sampling Rate	2.500000 MS/s
	Time / Pt	400.000000 ns	Sampling Mode	RealTime
	Pts / Div	250.0000 kS	Trigger Delay	0 ms
	Mode	Stop	Slope	Positive
Trigger	Type	Edge	Level	0.0 mV
	Source	C1	Coupling	DC