


Lab Notebook Entry from LeCroy DSO
DSO S/N: LCRY4203N20379
User: LeCroyUser
Time: 10/4/2016 6:29:04 AM

10/4/2016 6:29:04 AM

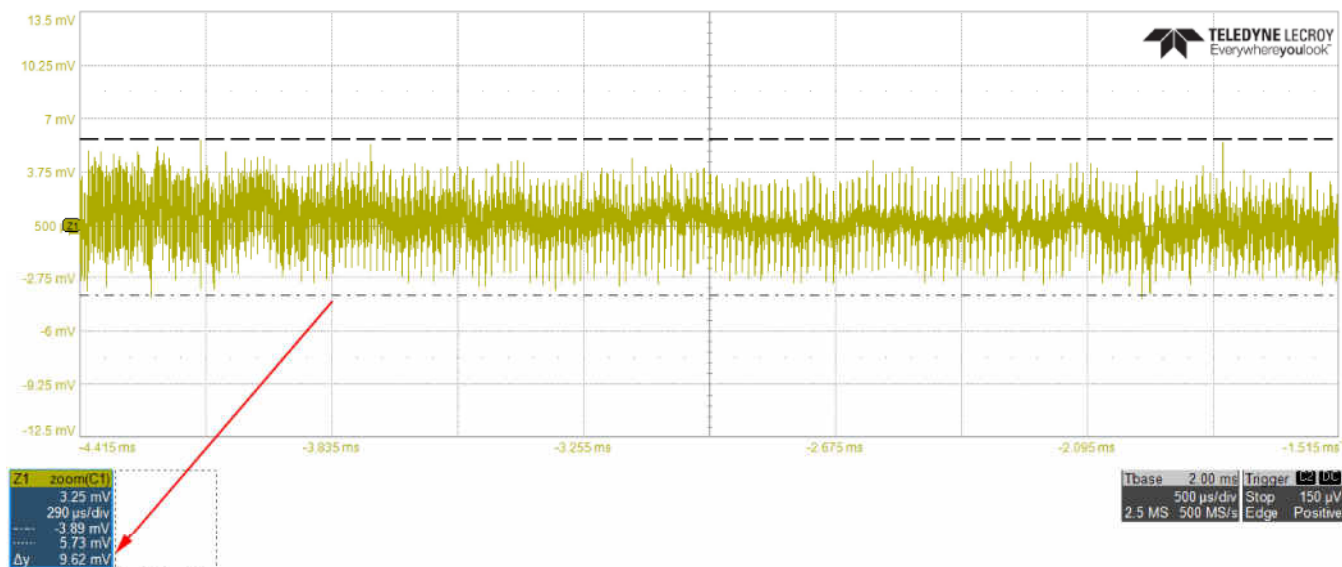

Channel Status

		C1
Vertical	V / Div	20.0 mV
	Offset	0.00 mV
	Coupling	AC1M Ω
	BW-Limit	20MHZ
	Probe	10
	Sweeps	1 #

Acquisition Status

Horizontal	Time / Div	500 μ s	Sampling Rate	500.000000 MS/s
	Time / Pt	2.000000 ns	Sampling Mode	RealTime
	Pts / Div	250.0000 kS	Trigger Delay	2.00 ms
Trigger	Mode	Stop	Slope	Positive
	Type	Edge	Level	150 μ V
	Source	C2	Coupling	DC