


Lab Notebook Entry from LeCroy DSO
DSO S/N: LCRY4203N20379
User: LeCroyUser
Time: 5/29/2017 11:13:55 PM

5/29/2017 11:13:55 PM

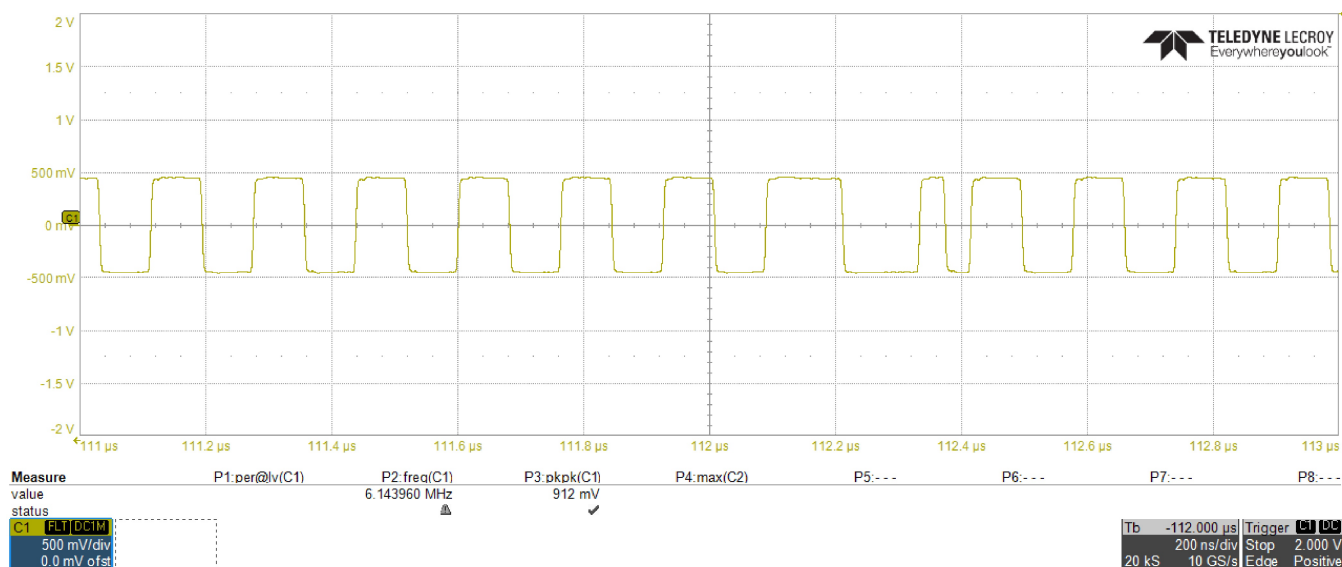

Channel Status

		C1
Vertical	V / Div	500 mV
	Offset	0.0 mV
	Coupling	DC1MΩ
	BW-Limit	1GHZ
	Probe	10
	Sweeps	1 #

Acquisition Status

Horizontal	Time / Div	200 ns	Sampling Rate	10.000000000 GS/s
	Time / Pt	100.000 ps	Sampling Mode	RealTime
	Pts / Div	2.0000 kS	Trigger Delay	-112.000 μs
	Mode	Stop	Slope	Positive
Trigger	Type	Edge	Level	2.000 V
	Source	C1	Coupling	DC