

## REFERENCES

- [1] D. A. Hill, "Plane wave integral representation for fields in reverberation chamber," *IEEE Trans. Electromagn. Compat.*, vol. 40, no. 3, pp. 209–217, Aug. 1998.
- [2] J. A. Stratton, *Electromagnetic Theory*. New York: McGraw-Hill, 1941, Sec. 7.7.
- [3] P. Corona, G. Ferrara, and M. Migliaccio, "A spectral approach for the determination of the reverberating chamber quality factor," *IEEE Trans. Electromagn. Compat.*, vol. 40, no. 2, pp. 145–153, May 1996.
- [4] M. Höjjer, "Maximum power available to stress onto the critical component in the equipment under test when performing a radiated susceptibility test in the reverberation chamber," *IEEE Trans. Electromagn. Compat.*, vol. 48, no. 2, pp. 372–384, May 2006.
- [5] P. Corona, G. Latmiral, and E. Paolini, "Performance and analysis of a reverberating enclosure with variable geometry," *IEEE Trans. Electromagn. Compat.*, vol. EMC-22, no. 1, pp. 2–5, Feb. 1980.
- [6] P. Corona and E. Piccioli, "Magnification factor for mode stirred chambers," presented at the Int. Symp. Electromagn. Compat., Washington, DC, Aug. 23–25, 1983.
- [7] P. Corona and G. Latmiral, "Approccio termodinamico allo studio di una camera riverberante elettromagnetica a geometria variabile", Estratto dal Volume Studi in Onore di Giuseppe Simeon, Istituto Universitario Navale, Napoli, Italy, 1978, pp. 309–319.
- [8] D. A. Hill, M. T. Ma, A. R. Ondrejka, B. F. Riddle, M. L. Crawford, and R. T. Johnk, "Aperture excitation of electrically large, lossy cavities," *IEEE Trans. Electromagn. Compat.*, vol. 36, no. 3, pp. 169–177, Aug. 1994.
- [9] R. E. Richardson Jr., "Mode-stirred chamber calibration factor, relaxation time, and scaling laws," *IEEE Trans. Electromagn. Compat.*, vol. 34, no. 4, pp. 573–580, Dec. 1985.

## Gas Discharge Tube Modeling With PSpice

Julio Guillermo Zola

**Abstract**—Gas discharge tubes (GDT)—sometimes named spark gaps (SGs)—are commonly used to suppress transients in many applications, from high-frequency communications to ac medium-power supply lines. The sharp GDT breakdown characteristics enable them to provide suitable transient suppression performance. A simple model of GDT for personal simulation program with integrated circuit emphasis (PSpice) simulation, based on theoretical triac behavior, is proposed in this correspondence. The comparison between real measured characteristics and the proposed model results in a suitable approach for the overvoltage transient response without typical problems of numerical convergence.

**Index Terms**—Overvoltage protection, simulation program with integrated circuit emphasis (SPICE), spark gaps (SGs).

## I. INTRODUCTION

Gas discharge tubes (GDTs), also called spark gaps (SGs), work based on an ionized gas discharge (inert gas or air) when a transient overvoltage is applied. At low values of applied voltage, a GDT acts as a high-value impedance (picofarad capacitance). Above a threshold

Manuscript received September 21, 2007; revised January 8, 2008, March 21, 2008, and June 20, 2008. First published October 28, 2008; current version published November 20, 2008.

The author is with the Department of Electronic Engineering, Faculty of Engineering, University of Buenos Aires, Paseo Colon 850 (C1063ACV) Buenos Aires, Argentina (e-mail: jzola@fi.uba.ar).

Digital Object Identifier 10.1109/TEM.2008.2004808

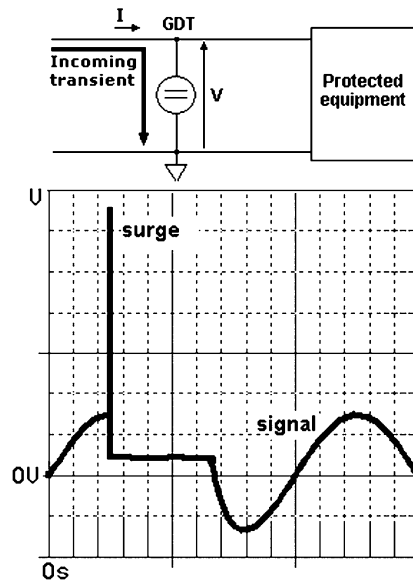
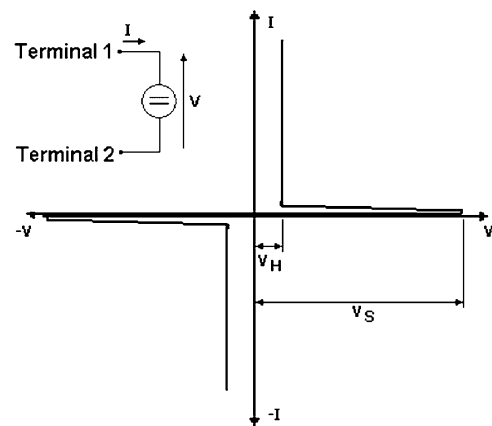


Fig. 1. Equipment protected with GDT.

Fig. 2.  $I$ - $V$  dc characteristic.

voltage, the GDT switches to a very low impedance state, presenting a negative resistance effect and clamping at a holdover voltage (threshold voltage), lower than the applied sparkover voltage.

When the voltage applied is lower than the threshold voltage, the GDT becomes nonconductive again. With these properties, GDTs are employed in electrical applications, such as power lines, communication lines, signal lines, and data transmission lines, to protect circuitry from transient overvoltages (damage caused by transient surge voltages that typically result from lightning strikes and equipment switching operations).

For protection purposes, GDTs are shunted with the system to be protected, between the signal line and ground (see Fig. 1), diverting the energy away from the sensitive equipment when overvoltages are applied. The potentially destructive energy of the incoming transient pulse is absorbed by the GDT, thereby protecting vulnerable circuit components and preventing potentially costly system damage [1].

For precise simulation, it is necessary to consider the dynamic properties of GDTs. During a low frequency pulse, the voltage across the GDT decreases quickly to the threshold value (see Fig. 2), similar to the theoretical triac behavior. This  $I$ - $V$  characteristic is the basis for the proposed model of the GDT.

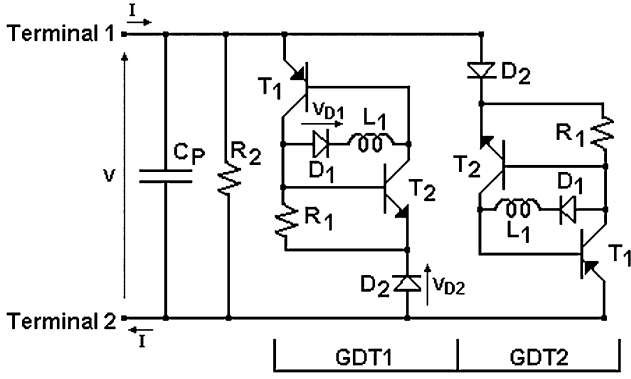


Fig. 3. Proposed model.

TABLE I  
EXAMPLE OF MODEL PARAMETERS EXTRACTION

SL1002A090: Device characteristics	SL1002A090: Model parameters
DC Voltage: 90V	$V_S = V_{BD1} + V_{BD2} = 90V$
Threshold Voltage: 50 V	$V_H = V_{BD2} = 50 V \Rightarrow V_{BD1} = 40 V$
Leakage Current: 100 nA (measured at 50V)	$R_2 = 50V / 100 nA = 500 M\Omega$
Capacitance: 1.2 pF	$C_P = 1.2 pF$
Dynamic Breakover Voltage: 360V	$V_{dS} = 360 V = V_S + L_1(\Delta I / \Delta t)$ $\Rightarrow 270 V \cong L_1(5 KA / 8 \mu s)$
Repetitive Impulse Discharge Current (8/20 $\mu s$ ): 5 KA	$\Rightarrow L_1 \cong 0.4 \mu H$
Voltage vs. Time Characteristic: Time response $\cong 300 ns$	$TF1 + TF2 = 300 ns$ $\Rightarrow TF1 = TF2 = 150 ns$
Glow-Arc transition Current: < 0.5 A	$R_1 = V_{jBE2} / 0.5 A = 1 \Omega$ $V_{jBE2} \cong 0.5 V$ is $T_2$ base-emitter junction voltage before to on state

A simple model of GDT for personal simulation program with integrated circuit emphasis (PSpice) simulation, based on theoretical triac behavior, is proposed in this correspondence. The parameters of the model, which are lower than current models of GDT, are extracted from electrical characteristics datasheets of GDT. This is suitable to build a model of a particular GDT quickly, and test by simulation the performance of GDT surge protection over the equipment to be protected. Behavior model is validated by measurement.

Since the model has been applied to GDT from different manufacturers, having different electrical characteristics, the repeatability of the proposed model is assured.

## II. BUILDING THE MODEL

The proposed model of the GDT for PSpice simulation, (Orcad-PSpice, Intusoft-Spice, or MicroCap-Spectrum) [2], is based on the triac model. Fig. 3 shows a circuit model, a half circuit GDT1 for dc and another half GDT2, for reverse current.

The transistors  $T_1$  and  $T_2$  are the triac bases. The dc sparkover voltage ( $V_S$ ) and threshold voltage ( $V_H$ ) are fixed for  $D_1$  and  $D_2$  reverse breakdown voltages ( $V_{BD1}$  and  $V_{BD2}$ , respectively)

$$V_S = V_{BD1} + V_{BD2} \quad V_H = V_{BD2}. \quad (1)$$

$R_1$  (glow current value) and  $R_2$  (isolated resistance) significantly help numerical convergence. Table I shows an example of model parameters extraction using datasheet values.

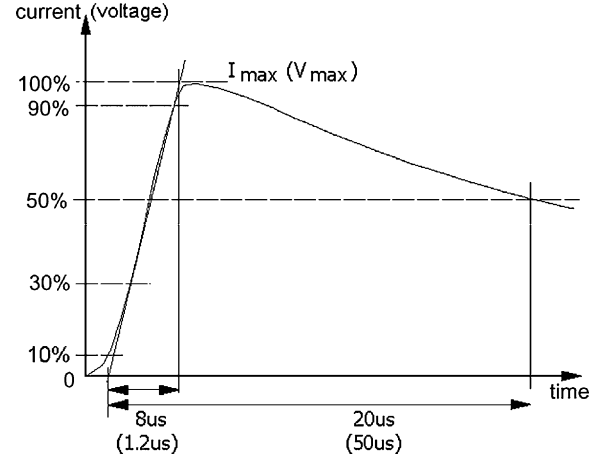


Fig. 4. Standard waveform.

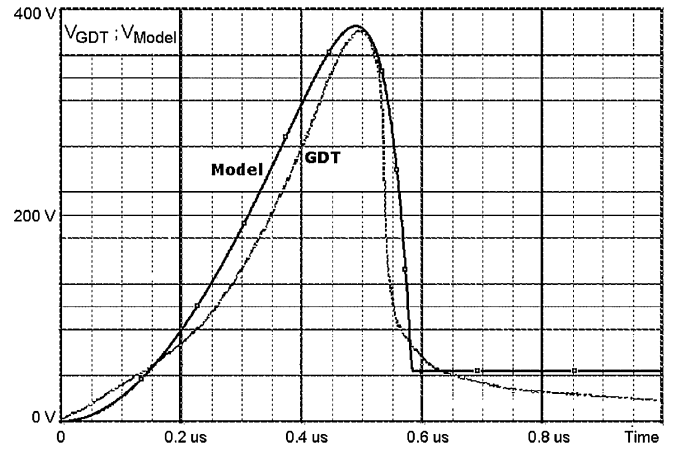



Fig. 5. GDT versus model response when a standard combination wave is applied.

On the other hand, the dynamic sparkover voltage (or dynamic breakover voltage)  $V_{dS}$  depends on the impulse voltage applied  $dV/dt$ . For example, most datasheets show dynamic breakover voltages at 100 V/ $\mu s$ . The maximum  $V_{dS}$  in these cases is higher than  $V_S$  (two or three times). The inductance  $L_1$  (0.1–1  $\mu H$ ) in series with  $D_1$  and the time parameter of bipolar junction transistors models  $TF$  (10–100 ns), take into account this dynamic response. The parallel capacitance  $C_P$  shows the behavior at nonconductive state.


## III. PROPOSED MODEL VERSUS MEASURED GDTs

Lightning, inductive load switching, or capacitor bank switching are often the sources of these overvoltage transients. The wave shape of a typical surge is similar to that of Fig. 4. The voltage surge is defined as a 1.2/50- $\mu s$  waveform, while the current surge is an 8/20- $\mu s$  waveform [3], [4]. Other standard current waveforms are 10/200, 10/1000  $\mu s$ , etc. [5].

Figs. 5 and 6 show the comparison between the time response for the proposed model, using Orcad-PSpice 9 [6], [7], and measured 90- and 230-V GDTs.

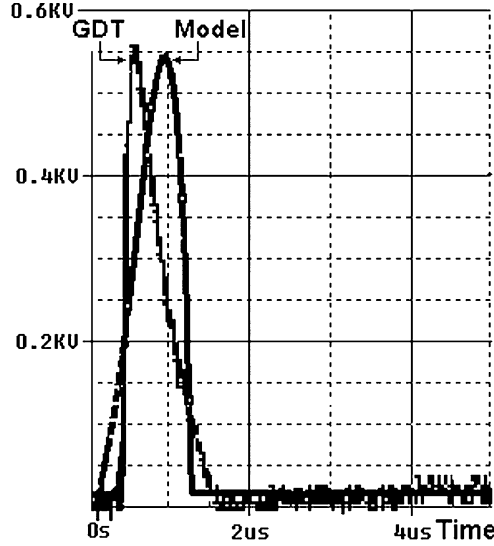

(a)

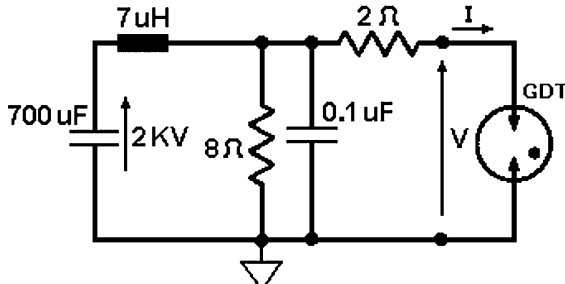

(b)

Fig. 6. (a) GDT versus model response to 1-kA 10/1000- $\mu$ s waveform. (b) Surge generator model.

Fig. 5 shows the voltage versus time characteristic of GDT SL1002A090, extracted from datasheets and the proposed model response, when a standard combination wave is applied.

The standard impulse of a combination waveform generator is characterized by the output voltage under open-circuit conditions and the output current under short-circuit conditions. The open-circuit voltage shall have a front time of 1.2  $\mu$ s and a time of half value of 50  $\mu$ s. The short-circuit current shall have a front time of 8  $\mu$ s and a time to half value of 20  $\mu$ s [8]. In this case, we have 20-kV 1.2/50- $\mu$ s open circuit and 5-KA 8/20- $\mu$ s short circuit.

Fig. 6(a) shows the GDT N81-A230X and the proposed model response when a 1-KA 10/1000- $\mu$ s waveform is applied. Fig. 6(b) shows the surge generator model used for simulation.

For this measurement, a surge generator (2-kV 1.2/3000- $\mu$ s open circuit and 1-KA 10/1000- $\mu$ s short circuit) and a digital scope Tektronix model TDS1002 (60 MHz, 1 GSamples/s and 10 $\times$  probe) were used (see Fig. 7).

Note that the measured voltage in Fig. 6 has a negative zero crossing. This is due to normal sample error at very low voltages values that are neglected for the measurement.

The resistors of surge generator in Fig. 7, specified in IEEE Standard C62.31,  $R_1$  (impulse-shaping resistor) and  $R_2$  (impulse-shaping and current-limiting resistor) have values between 8 to 10 and 1 to 2  $\Omega$ , respectively. The voltage of GDT is reduced 100 times at the scope input (see Fig. 7).

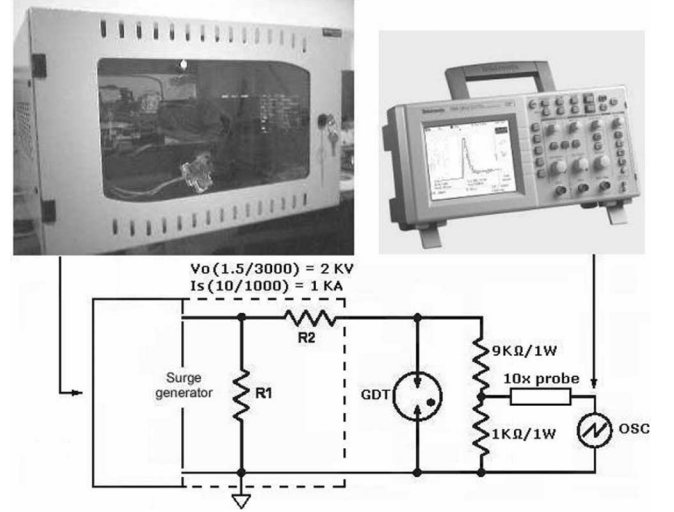


Fig. 7. Measurement diagram.

TABLE II  
NETLISTS COMPARISON

Current model	Proposed model
.subckt sprkpg 1 2 EB_C 6 0 value={if(abs(v(1,2))>90 +  abs(l(vs))>4m,12,0)} DT1 6 7 1N4148 CT1 7 0 .25U RT1 7 0 50 SB 1 3 7 0 C_S .model C_S vswitch Voff=0 Von=10 + Ron=500u Roff=50meg VS 5 2 EA_C 8 0 value={if(abs(l(vs))>0.2,12,0)} DT2 8 9 1N4148 CT2 9 0 .1U RT2 9 0 50 SA 3 10 9 0 C_S D1 3 4 GW D2 5 4 GW .model GW d bv=20 is=1u rs=5u ibv=10u D3 10 11 ARC D4 5 11 ARC .model ARC d bv= 50 is=1U rs=5u ibv=10U .model 1N4148 d is=2.7n n=1.8 rs=.6 Vj=.5 + ikf=44m xti=3 eg=1.11 cjo=4p m=.33 fc=.5 + isr=1.6n nr=2 bv=100 ibv=100u tt=11.5n .ends	.subckt sprkpg 1 2 RP 1 2 .5G CP 2 1 1.2P R1 3 4 1 D1 3 100 D1 L1 100 5 .4U Q1 3 5 1 P Q2 5 3 4 N D2 2 4 D2 .model D1 D bv=40 .model D2 D bv=50 .model P pnp tf=.15U .model N npn tf=.15U R10 30 40 1 D10 30 200 D1 L10 200 50 .4U Q10 30 50 2 P Q20 50 30 40 N D20 1 40 D2 .ends

#### IV. CONCLUSION

The triac-based GDT model allows us to obtain a good fit to measured characteristics with few parameters and an improvement in numerical convergence.

Table II shows an example of PSpice netlists: current model (used in [9]–[11]) and proposed model (used in [12]).

The following facts should be noted.

- 1) The number of parameters to be preset to create the new model is reduced.
- 2) The proposed model does not use switches. In the current models, the switch parameters,  $R_{ON}$ ,  $R_{OFF}$ , and its ratio  $R_{ON}/R_{OFF}$ , must be carefully selected to avoid problems of numerical convergence.

## REFERENCES

- [1] T. Basso, T. Sinard, and T. France. (1997, Jul. 3). Spice model simulates spark-gap arrestor—EDN access. [Online]. Available: [www.reed-electronics.com/ednmag/archives/1997/070397/14di\\_06.htm](http://www.reed-electronics.com/ednmag/archives/1997/070397/14di_06.htm)
- [2] G. Massobrio and P. Antognetti, *Semiconductor Device Modeling With SPICE*. New York: McGraw-Hill, 1993.
- [3] *Lightning Protection, NZS/AS 1768 Appendix D*, Australian Standard, 1991.
- [4] *Test Methods for Low-Voltage Gas-Tube Surge-Protective Device Components*, IEEE Standard 62.31, 2006.
- [5] R. B. Standler, "Equations for some transient overvoltage test waveforms," *IEEE Trans. Electromagn. Compat.*, vol. 30, no. 1, pp. 69–71, Feb. 1988.
- [6] Cadence PSpice. (2000). [Online]. Available: <http://www.cadence.com/orcad/index.html>.
- [7] J. G. Zola, "Simple model of metal oxide varistor for PSpice simulation," *IEEE Trans. Comput.-Aided Design Integr. Circuits Syst.*, vol. 23, no. 10, pp. 1491–1494, Oct. 2004.
- [8] *Recommended Practice on Surge Testing for Equipment Connected to Low-Voltage (1000 V and Less) AC Power Circuits*, IEEE Standard 62.45, 2002.
- [9] A. Larsson, V. Scuka, K. Borgeest, and J. L. ter Haseborg, "Numerical simulation of gas discharge protectors—A review," *IEEE Trans. Power Del.*, vol. 14, no. 2, pp. 405–410, Apr. 1999.
- [10] B. Vahidi and J. Beiza, "Using PSpice in teaching impulse voltage testing of power transformers to senior undergraduate students," *IEEE Trans. Educ.*, vol. 48, no. 2, pp. 307–312, May 2005.
- [11] S. Bonisch and W. Kalkner, "Measurement and simulation of the behavior of a short spark gap used as ESD protection device," in *Proc. IEEE Int. Symp. Electromagn. Compat.*, Aug. 18–22, 2003, vol. 1, pp. 37–42.
- [12] E. Mariani, C. Piaggio, and J. Zola, "Modelling the TT low voltage distribution system in rural zones of Argentina under the effect of lightning," presented at the 9th Int. Symp. Lightning Protection, Foz do Iguazu, Brazil, Nov. 26–30, 2007.